



ALCOHOL BREATH TEST

Accuracy over 98% / Mas del 98% de precision / Genauigkeit über 98% / Précision plus de 98% / Affidabilità: oltre il 98%

EN: Wait 20 minutes after alcohol consumption before using this alcohol test.
ES: Espere 20 minutos despues de consumir alcohol antes de usar esta prueba de alcohol.
DE: Nach alkoholgenuss 20 minuten bis zum testbeginn warten
FR: Veuillez attendre 20 minutes après avoir consommé de l'alcool avant de faire cet éthylotest
IT: Prima di eseguire il test aspettare 20 Minuti dall'ultima assunzione di alcol



EN: Press firmly on both ends of the tube to break the security seal.
ES: Presione firmemente en ambos extremos del tubo para romper el precinto de seguridad.
DE: Auf beide enden des röhrchens fest drücken, um das sicherheitssiegel aufzubrechen.
FR: Appuyez fermement sur les deux extrémités du tube pour briser le sceau de sécurité
IT: Premere in modo deciso su ambo i lati del tubo per infrangere il sigillo di sicurezza



ALCOHOL BREATH TEST

Accuracy over 98% / Mas del 98% de precision / Genauigkeit über 98% / Précision plus de 98% / Affidabilità: oltre il 98%

EN: Wait 20 minutes after alcohol consumption before using this alcohol test.
ES: Espere 20 minutos despues de consumir alcohol antes de usar esta prueba de alcohol.
DE: Nach alkoholgenuss 20 minuten bis zum testbeginn warten
FR: Veuillez attendre 20 minutes après avoir consommé de l'alcool avant de faire cet éthylotest
IT: Prima di eseguire il test aspettare 20 Minuti dall'ultima assunzione di alcol



EN: Press firmly on both ends of the tube to break the security seal.
ES: Presione firmemente en ambos extremos del tubo para romper el precinto de seguridad.
DE: Auf beide enden des röhrchens fest drücken, um das sicherheitssiegel aufzubrechen.
FR: Appuyez fermement sur les deux extrémités du tube pour briser le sceau de sécurité
IT: Premere in modo deciso su ambo i lati del tubo per infrangere il sigillo di sicurezza



ALCOHOL BREATH TEST

Accuracy over 98% / Mas del 98% de precision / Genauigkeit über 98% / Précision plus de 98% / Affidabilità: oltre il 98%

EN: Wait 20 minutes after alcohol consumption before using this alcohol test.
ES: Espere 20 minutos despues de consumir alcohol antes de usar esta prueba de alcohol.
DE: Nach alkoholgenuss 20 minuten bis zum testbeginn warten
FR: Veuillez attendre 20 minutes après avoir consommé de l'alcool avant de faire cet éthylotest
IT: Prima di eseguire il test aspettare 20 Minuti dall'ultima assunzione di alcol



EN: Press firmly on both ends of the tube to break the security seal.
ES: Presione firmemente en ambos extremos del tubo para romper el precinto de seguridad.
DE: Auf beide enden des röhrchens fest drücken, um das sicherheitssiegel aufzubrechen.
FR: Appuyez fermement sur les deux extrémités du tube pour briser le sceau de sécurité
IT: Premere in modo deciso su ambo i lati del tubo per infrangere il sigillo di sicurezza



ALCOHOL BREATH TEST

Accuracy over 98% / Mas del 98% de precision / Genauigkeit über 98% / Précision plus de 98% / Affidabilità: oltre il 98%

EN: Wait 20 minutes after alcohol consumption before using this alcohol test.
ES: Espere 20 minutos despues de consumir alcohol antes de usar esta prueba de alcohol.
DE: Nach alkoholgenuss 20 minuten bis zum testbeginn warten
FR: Veuillez attendre 20 minutes après avoir consommé de l'alcool avant de faire cet éthylotest
IT: Prima di eseguire il test aspettare 20 Minuti dall'ultima assunzione di alcol



EN: Press firmly on both ends of the tube to break the security seal.
ES: Presione firmemente en ambos extremos del tubo para romper el precinto de seguridad.
DE: Auf beide enden des röhrchens fest drücken, um das sicherheitssiegel aufzubrechen.
FR: Appuyez fermement sur les deux extrémités du tube pour briser le sceau de sécurité
IT: Premere in modo deciso su ambo i lati del tubo per infrangere il sigillo di sicurezza



EN: Blow into the tube for 10 seconds in the direction of the arrows and then repeat (2 x 10 sec).
ES: Soplo en el tubo durante 10 segundos en la dirección de la flecha y luego repita dos veces mas durante 10 segundos.
DE: 10 sekunden lang in das röhrrchen, in richtung des pfeils blasen, danach wiederholen (2 x 10 sek.).
FR: Soufflez dans le tube pendant 10 secondes en suivant la direction des flèches puis répétez cette action (2 x 10s).
IT: Soffiare nel tubo per 10 secondi secondo la direzione della freccia. Soffiare una seconda volta per altri 10 secondi


EN: After 2-4 minutes compare your result with the scale on the tube.
ES: Despues de 2 - 4 minutos compare su resultado con la escala que se indica en el tubo.
DE: Nach 2 - 4 minuten das ergebnis mit der skala auf dem röhrrchen vergleichen.
FR: Après 2-4 minutes, comparez votre résultat avec le nuancier sur le tube.
IT: Dopo 2-4 minuti verificare il risultato con la scala presente sul tubo

Best Before / Consumase Antes De / Mindestens Haltbar Bis / Préférence avant / Da consumarsi preferibilmente entro :

08/2017

Manufactured By: Test&Drive, HURTOWNIK Group, ul. Dekoracyjna 3, 65-155 Zielona Góra, Poland.

Distributed in the UK by: Home Health UK Ltd, Unit 11, Peerglow Industrial Estate, Olds Approach, Watford, Herts, WD18 9SR. Email: info@homehealth-uk.com, Website: www.homehealth-uk.com

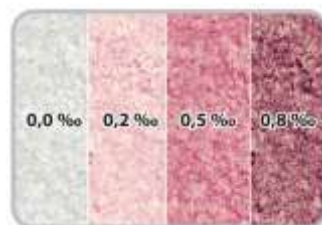

Version 1.3 01.08.15

EN: Blow into the tube for 10 seconds in the direction of the arrows and then repeat (2 x 10 sec).
ES: Soplo en el tubo durante 10 segundos en la dirección de la flecha y luego repita dos veces mas durante 10 segundos.
DE: 10 sekunden lang in das röhrrchen, in richtung des pfeils blasen, danach wiederholen (2 x 10 sek.).
FR: Soufflez dans le tube pendant 10 secondes en suivant la direction des flèches puis répétez cette action (2 x 10s).
IT: Soffiare nel tubo per 10 secondi secondo la direzione della freccia. Soffiare una seconda volta per altri 10 secondi



EN: After 2-4 minutes compare your result with the scale on the tube.
ES: Despues de 2 - 4 minutos compare su resultado con la escala que se indica en el tubo.
DE: Nach 2 - 4 minuten das ergebnis mit der skala auf dem röhrrchen vergleichen.
FR: Après 2-4 minutes, comparez votre résultat avec le nuancier sur le tube.
IT: Dopo 2-4 minuti verificare il risultato con la scala presente sul tubo

Best Before / Consumase Antes De / Mindestens Haltbar Bis / Préférence avant / Da consumarsi preferibilmente entro :

08/2017

Manufactured By: Test&Drive, HURTOWNIK Group, ul. Dekoracyjna 3, 65-155 Zielona Góra, Poland.

Distributed in the UK by: Home Health UK Ltd, Unit 11, Peerglow Industrial Estate, Olds Approach, Watford, Herts, WD18 9SR. Email: info@homehealth-uk.com, Website: www.homehealth-uk.com

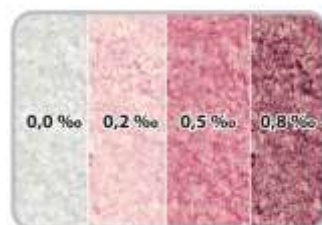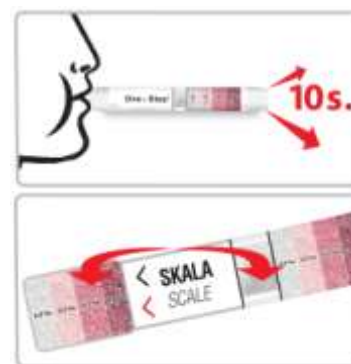

Version 1.3 01.08.15

EN: Blow into the tube for 10 seconds in the direction of the arrows and then repeat (2 x 10 sec).
ES: Soplo en el tubo durante 10 segundos en la dirección de la flecha y luego repita dos veces mas durante 10 segundos.
DE: 10 sekunden lang in das röhrrchen, in richtung des pfeils blasen, danach wiederholen (2 x 10 sek.).
FR: Soufflez dans le tube pendant 10 secondes en suivant la direction des flèches puis répétez cette action (2 x 10s).
IT: Soffiare nel tubo per 10 secondi secondo la direzione della freccia. Soffiare una seconda volta per altri 10 secondi



EN: After 2-4 minutes compare your result with the scale on the tube.
ES: Despues de 2 - 4 minutos compare su resultado con la escala que se indica en el tubo.
DE: Nach 2 - 4 minuten das ergebnis mit der skala auf dem röhrrchen vergleichen.
FR: Après 2-4 minutes, comparez votre résultat avec le nuancier sur le tube.
IT: Dopo 2-4 minuti verificare il risultato con la scala presente sul tubo

Best Before / Consumase Antes De / Mindestens Haltbar Bis / Préférence avant / Da consumarsi preferibilmente entro :

08/2017

Manufactured By: Test&Drive, HURTOWNIK Group, ul. Dekoracyjna 3, 65-155 Zielona Góra, Poland.

Distributed in the UK by: Home Health UK Ltd, Unit 11, Peerglow Industrial Estate, Olds Approach, Watford, Herts, WD18 9SR. Email: info@homehealth-uk.com, Website: www.homehealth-uk.com

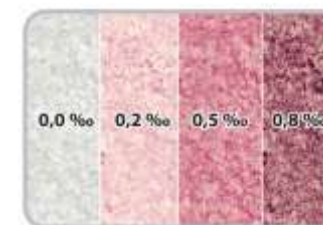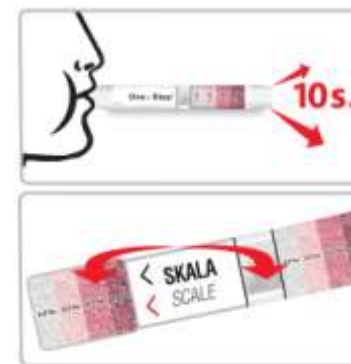

Version 1.3 01.08.15

EN: Blow into the tube for 10 seconds in the direction of the arrows and then repeat (2 x 10 sec).
ES: Soplo en el tubo durante 10 segundos en la dirección de la flecha y luego repita dos veces mas durante 10 segundos.
DE: 10 sekunden lang in das röhrrchen, in richtung des pfeils blasen, danach wiederholen (2 x 10 sek.).
FR: Soufflez dans le tube pendant 10 secondes en suivant la direction des flèches puis répétez cette action (2 x 10s).
IT: Soffiare nel tubo per 10 secondi secondo la direzione della freccia. Soffiare una seconda volta per altri 10 secondi



EN: After 2-4 minutes compare your result with the scale on the tube.
ES: Despues de 2 - 4 minutos compare su resultado con la escala que se indica en el tubo.
DE: Nach 2 - 4 minuten das ergebnis mit der skala auf dem röhrrchen vergleichen.
FR: Après 2-4 minutes, comparez votre résultat avec le nuancier sur le tube.
IT: Dopo 2-4 minuti verificare il risultato con la scala presente sul tubo

Best Before / Consumase Antes De / Mindestens Haltbar Bis / Préférence avant / Da consumarsi preferibilmente entro :

08/2017

Manufactured By: Test&Drive, HURTOWNIK Group, ul. Dekoracyjna 3, 65-155 Zielona Góra, Poland.

Distributed in the UK by: Home Health UK Ltd, Unit 11, Peerglow Industrial Estate, Olds Approach, Watford, Herts, WD18 9SR. Email: info@homehealth-uk.com, Website: www.homehealth-uk.com

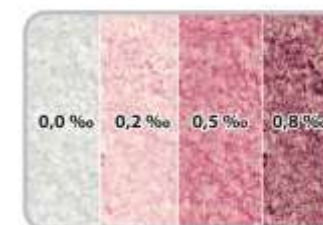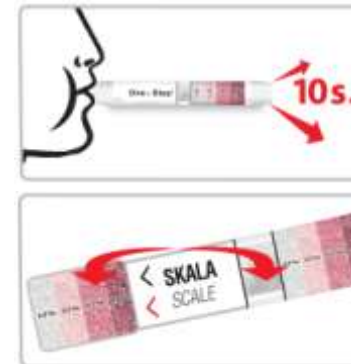

Version 1.3 01.08.15